

Approved by FDA & CE



QBit 9

Smart Ultrasound



CHISON | **20** Years Anniversary
Value Beyond Imaging | 1996 - 2016

Ergonomics



19" LED up & down
90° foldable



Depth View




The LED screen can be rotated left and right $-90^{\circ}\sim 90^{\circ}$ allow different viewing angles of patients and operators

Stereo audio system



Backlit keys

Floating keyboard with left/right rotation $-45^{\circ}\sim 45^{\circ}$, up/down height adjustment 0cm~15cm



Hero Kit

Innovative service solution
Quick • Easy • Reliable • Affordable



Removable dust filter.

Built-in battery 80min (option)



Print paper face to the front, for easy access.

35.6 cm
Small foot print

Four wheels with locks



Virtual HD

- The latest innovation in real-time 4D with powerful imaging engine.
- Greatly strengthen the bond between mother and fetus. With moveable virtual light source.


Women's healthcare




BPD, B Mode



Umbilical Cord, C Mode

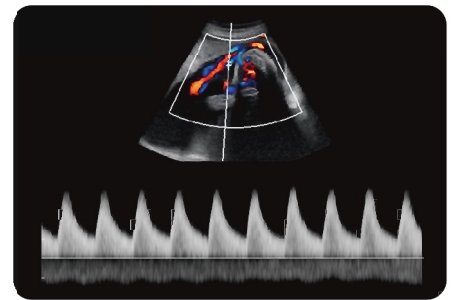

Umbilical Cord, PW Mode

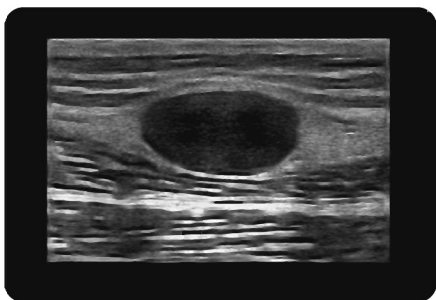


Breast Cyst, B Mode




Uterus, B Mode




Early Pregnancy, B Mode

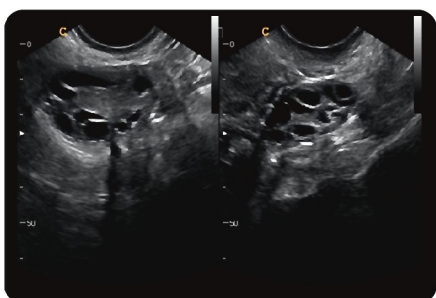

Ovary, 2B Mode

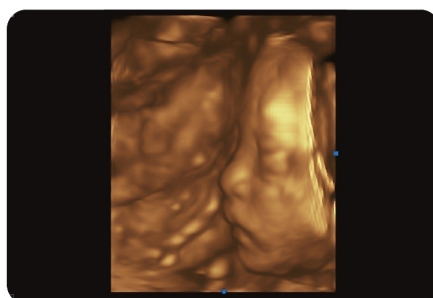


Fetal Face, 4D Mode

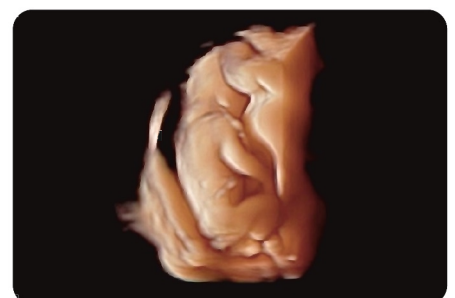

Fetal Body, Virtual HD


FHI

An innovative harmonic technology that using different transmission and receiving methods for different body sized patients, to maximize the resolution without losing the penetration. Better than traditional THI and phased harmonic which compromise the penetration.




Cardiology Performance


QBit 9

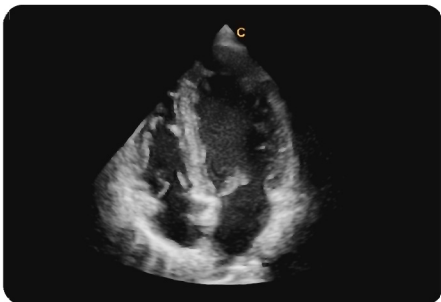


Apical Four Chambers, FHI Mode

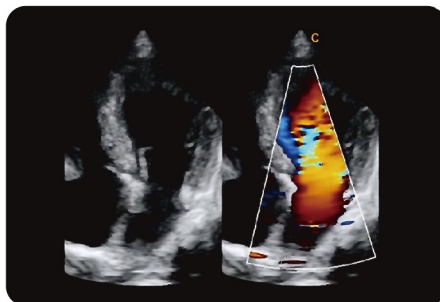


Apical Four Chambers, C Mode

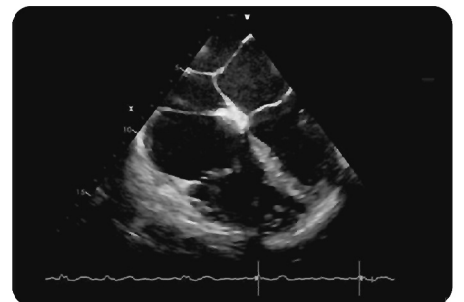


Cardiac, TEE

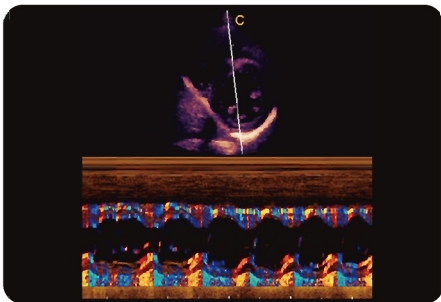

Papillary Muscle Short Axis, TDI M Mode

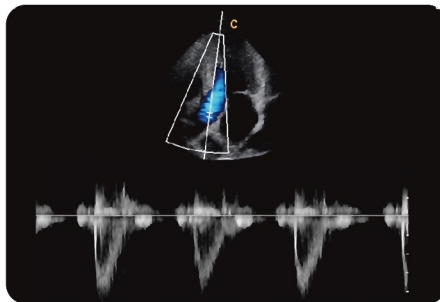

Aortic Valve, PW Mode

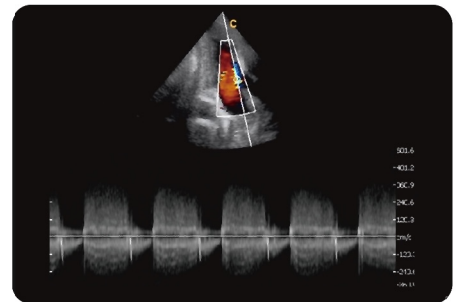



AV Regurgitation, CW Mode

State-Of-Art Performance



PISA

PISA is Proximal Isovelocity Surface Area, a method to look at flow convergence, to calculate severity of MR/TR/PR.

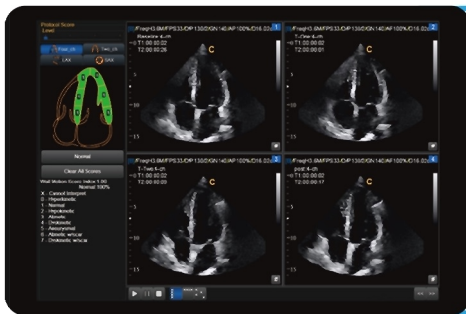
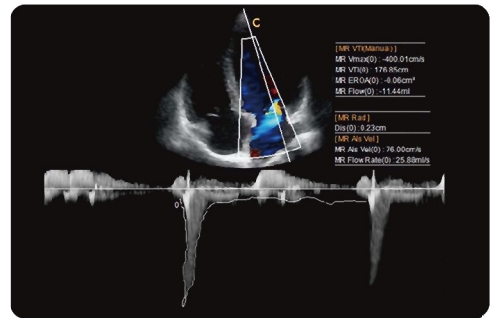


StressEcho

An echocardiogram is a painless, harmless test that uses high frequency sound waves to examine the heart's anatomy function.

Tissue Doppler Imaging (TDI)

Tissue Doppler imaging is a novel echocardiography technique that directly measures myocardial velocity. Systolic TD measurements assess left and right ventricular myocardial contractile function. Diastolic TD values reflect myocardial relaxation.

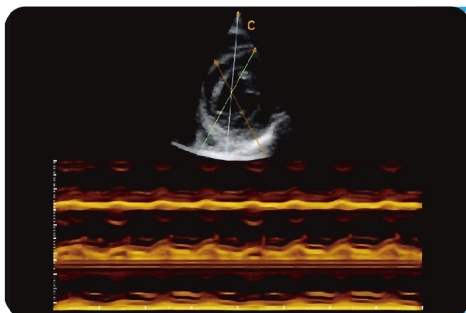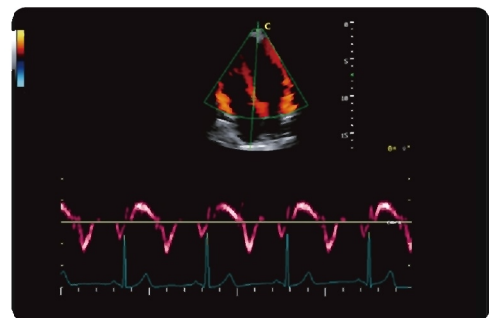

Free Steering M Mode


The cursor line can be rotated in 360 degree and placed at the desired position up to 3 lines can be used for simultaneous measurements.

Advanced

Technologies


Q-image

- These innovative algorithms have strengthened the image enhancement results significantly.
- Advanced chipset is used to ensure fast frame rate.

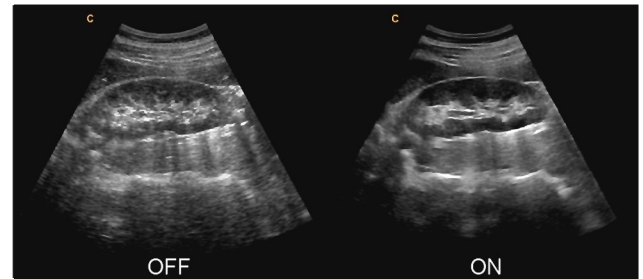


Q-beam

- Compared to the traditional dual-beam, Qbit uses quad-beam to receive signal, thus doubles the volume of signal received as well as the frame rate.
- Higher frame rate ensures better diagnostic confidence and efficiency.

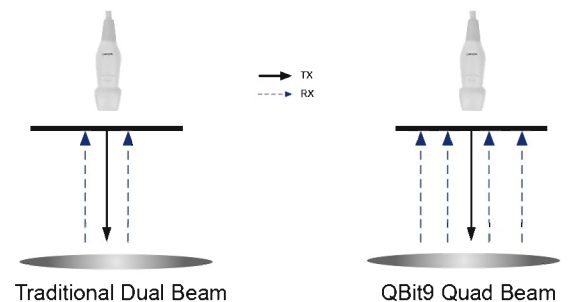


Q-flow

- This adaptive color detection technology can automatically adjust the criteria of color and noise assessment in different tissues.
- As a result, color sensitivity of low-velocity flow is greatly enhanced.

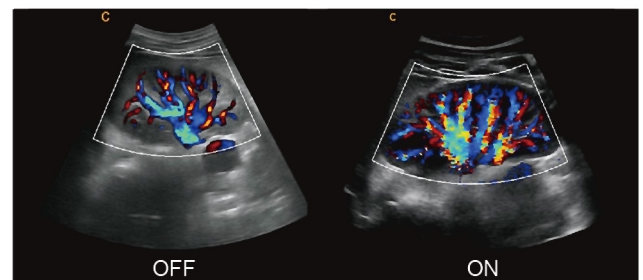

X-contrast


- Adjust the contrast resolution to three levels according to the tissue difference.
- Activated by one key: Enhance, Normal, Suppress.

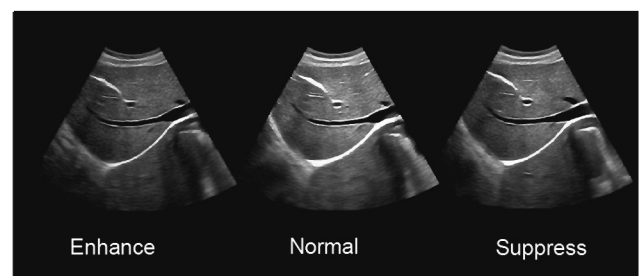




General Imaging

Small Parts

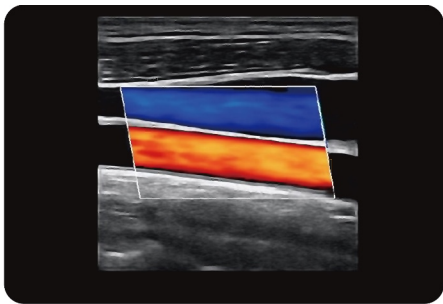


Carotid, C Mode

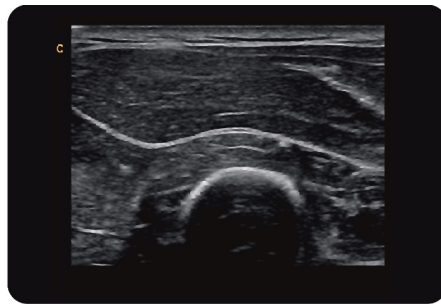


Elbow Point, B Mode




Thyroid, B Mode

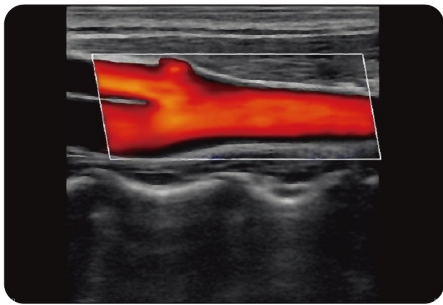


Carotid, C Mode

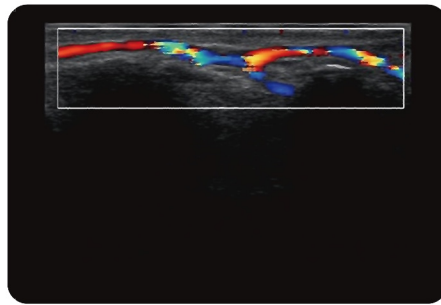


Finger Vessel, C Mode

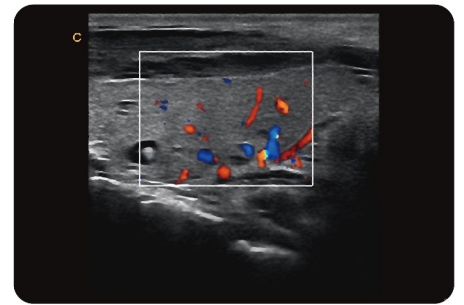


Thyroid, C Mode

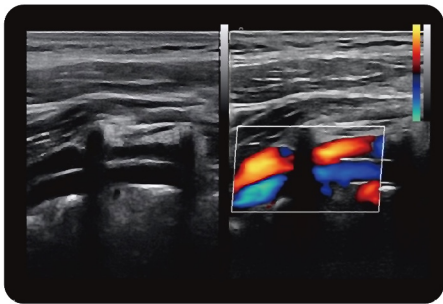


Vertebral Artery, 2B Mode

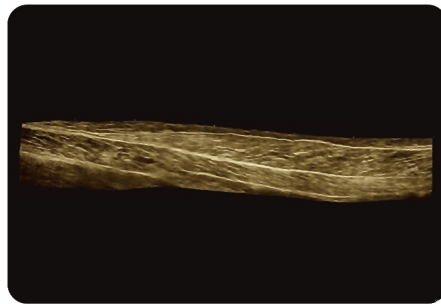

Muscle, Real Time Panoramic

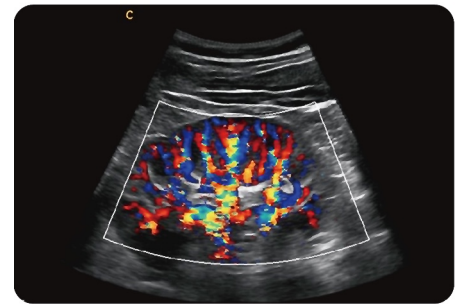

Kidney, C Mode





QBit 9

Smart Ultrasound



2.0MHz-6.8MHz Convex
D3C60L



4.0MHz-15.0MHz Linear
D7L40L



7.0MHz-18.0MHz(With FHI) Linear
D12L40L



4.0MHz-15.0MHz Linear
D7L60L-60mm



4.0MHz-12.0MHz Transvaginal
D6C12L



1.5MHz-5.3MHz Phased array
D3P64L



4.0MHz-15.0MHz Transvaginal
D7C10L



4.0MHz-15.0MHz Trans Rectal
D7L40L-REC



2.0MHz-6.8MHz Volume
V4C40L



2.0MHz-6.8MHz Micro-Convex
D3C20L




2.0MHz-8.0MHz Phased array
D6P64L



4.0MHz-12.0MHz Micro-Convex
D6C15L



4.0MHz-10.7MHz Micro-Convex
D5C20L



4.0MHz-6.0MHz Tee(Adult)
T5P64L



4.0MHz-6.0MHz Tee(Pediatric)
MT5P48L



1.5MHz-2.5MHz Pencil
D2D16L



4.0MHz-10.7MHz Linear
D7L30L

CHISON MEDICAL IMAGING CO., LTD.

Sales & Service Contact Address:

No. 9 Xin Hui Huan Road, New District, Wuxi, Jiang Su Province, China214028

TEL: 0086-510-85310593 / 85310937 FAX: 0086-510-85310726 EMAIL: export@chison.com.cn

We reserve the right to make changes to this catalogue without prior notice
Please contact our local dealer for the latest information.

EQBit 9-160104